

Human GFAP Ready-To-Use IHC Kit

Cat. No.: IHC0101H

Sample Type: FFPE tissue

Size: 50T (including a control slide)

Storage and Stability: Please store components at the temperatures indicated on the individual tube labels. The kit is stable for 6 months from the date of receipt.

General Information

| Number | Component | Size | Concentration | Storage |
|--------|---|---------|---------------|---------|
| 1 | PBS Buffer (powder) | 2 L×2 | 20x | RT |
| 2 | Antigen Retrieval Buffer | 20 ml | 100x | 2-8°C |
| 3 | Endogenous Peroxidase Blocking Buffer | 3 ml | RTU | 2-8°C |
| 4 | Blocking Buffer | 3 ml | RTU | 2-8°C |
| 5 | Primary Antibody (Human GFAP Rabbit pAb) | 6 ml | RTU | 2-8°C |
| 6 | Secondary Antibody (HRP-Goat anti-Rabbit IgG pAb) | 6 ml | RTU | 2-8°C |
| 7 | Chromogen Component A | 0.3 ml | RTU | -20°C |
| 8 | Chromogen Component B | 0.3 ml | RTU | -20°C |
| 9 | Counter Staining Reagent | 5 ml | RTU | RT |
| 10 | Mounting Media | 5 ml | RTU | RT |
| 11 | Control slide (Human brain) | 1 slide | RTU | RT |
| 12 | Datasheet | 1 copy | | |


Background

GFAP (Glial fibrillary acidic protein) is a member of the class III intermediate filament protein family. GFAP is heavily and specifically expressed in astrocytes and certain astroglia of the central nervous system, in satellite cells of peripheral ganglia, and in non-myelinating Schwann cells of peripheral nerves. In addition, neural stem cells strongly express GFAP. Antibodies to GFAP are very useful as markers of astrocytic cells. In addition, many types of brain tumor, presumably derived from astrocytic cells, heavily express GFAP. GFAP is also found in the lens epithelium, Kupffer cells of the liver, in some cells in salivary tumors and has been reported in erythrocytes. GFAP is used as a marker to distinguish astrocytes from other glial cells during development. Mutations in this gene cause Alexander disease, a rare disorder of astrocytes in the central nervous system. Alternative splicing of the GFAP gene results in multiple transcript variants encoding distinct isoforms.

Synonyms

Astrocyte Marker; FLJ45472; GFAP; Glial Fibrillary Acidic Protein; Intermediate filament protein; GFAP_HUMAN.

Validation Data

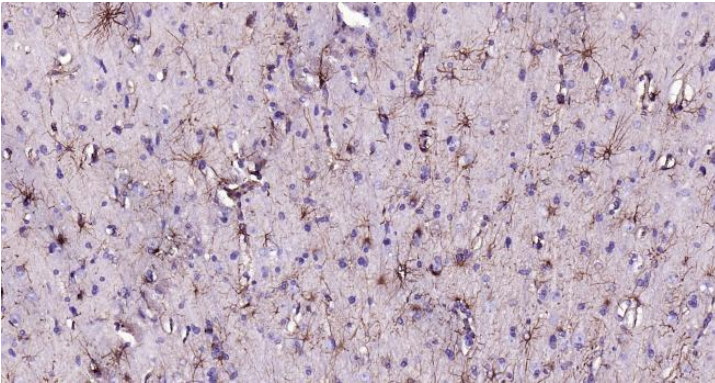

Immunohistochemical analysis of paraffin embedded human glioma tissue slide using IHC0101H (Human GFAP IHC Kit).

Immunohistochemistry Protocol

1. Deparaffinization And Rehydration

Immerse slides in fresh xylene for 15 minutes and then repeat two more times using separate containers. Immerse slides sequentially in 100%, 95%, 90%, 80%, and 70% ethanol solutions for 5 minutes each. Rinse slides 3 times with distilled water for 5 minutes each.

2. Antigen Retrieval

Add 100 × **Antigen Retrieval Buffer** into distilled water to prepare a 1 × solution. Boil slides in 1 × solution at 95°C-100°C for 15 minutes. Move the slides to 1 × solution at room temperature (RT) and allow them to stand for 20 minutes. Rinse 3 times with **PBS Buffer** (dissolve the powder in 2L distilled water) for 5 minutes each.

3. Block Endogenous Peroxidase

Drain the liquid off the slides and then use a hydrophobic IHC pen to draw circles on the slides around tissue sections. Add 2-4 drops of **Endogenous Peroxidase Blocking Buffer** directly on slides, covering the whole tissue and block slides for 15 minutes at RT. Rinse 3 times with **PBS Buffer** for 5 minutes each.

4. Serum Blocking

Block with 2-4 drops of **Blocking Buffer** for 20 minutes at RT.

5. Primary Antibody Incubation

Drain blocking buffer from slides. Incubate slides with 2-4 drops of **Human GFAP Rabbit pAb** overnight at 4°C or 1-2 hours at RT. Rinse 3 times with **PBS Buffer** for 5 minutes each.

6. Secondary Antibody Incubation

Incubate slides with 2-4 drops of **HRP-Goat anti-Rabbit IgG pAb** for 1-2 hours at RT. Rinse slides 3 times with **PBS Buffer** for 5 minutes each.

7. Signal Development

Remove residual liquid around the tissue section. Add 50ul fresh **DAB Buffer (Chromogen Component A : Chromogen Component B : PBS Buffer=1:1:18)** to cover the tissue. Monitor the reaction under the microscope until a brown color is visible (approximate 3-5 minutes at RT). Stop reaction immediately by rinsing with distilled water. Rinse slides 3 times with distilled water for 5 minutes each.

8. Counterstain

Counterstain with an appropriate amount of **Counter Staining Reagent** for 3-5 minutes at RT. Rinse slides with distilled water for 5 minutes. Use 2-4 drops of **Differentiation reagent** to cover the tissue for 30 seconds. Rinse slides twice with distilled water for 5 minutes each.

9. Dehydration Sheet

Immerse slides sequentially in 70%, 80%, 90%, 95%, and 100% ethanol for 5 minutes each at RT. Immerse slides in 2 changes of fresh xylene, 15 minutes each. Drop some **Mounting Media** on the tissue. Mount coverslips.

Notes

1. The positive control slide provided in the kit allows you to be sure that the experimental set-up is working properly.
2. Do not allow slides to dry at any time during this procedure.
3. Please don't replace the matching reagents in this product with other manufacturers' products.
4. As DAB is a carcinogen, please take necessary precautions.
5. PBS (reagent 1) can be stored for one week at 4°C after preparation; The antigen retrieval buffer (1× reagent 2) and the chromogenic agent (the mixture of reagents 7 and 8) should be prepared right before each assay.

Please cite this product as "IHC0101H, Bioss Antibodies". Citation example: "Human tissue sections using Human GFAP IHC Kit (IHC0101H, Bioss Antibodies) were stained for GFAP according to the manufacturer's instructions."

Human GFAP Ready-To-Use IHC Kit

人胶质纤维酸性蛋白即用型免疫组化试剂盒

产品货号: IHC0101H

样本类型: FFPE 组织切片

产品规格: 50T (包含一个对照切片)

保存条件: 见下表。有效期 6 个月。

产品组分及规格

| 编号 | 组分 | 规格 | 浓度 | 储存 |
|----|-----------------------------------|--------|------|------|
| 1 | PBS 缓冲液 (干粉) | 2 L×2 | 20x | 室温 |
| 2 | 抗原修复缓冲液 | 20 ml | 100x | 2-8℃ |
| 3 | 内源性过氧化物酶阻断剂 | 3 ml | RTU | 2-8℃ |
| 4 | 封闭工作液 | 3 ml | RTU | 2-8℃ |
| 5 | 一抗 (Human GFAP Rabbit pAb) | 6 ml | RTU | 2-8℃ |
| 6 | 二抗 (HRP-Goat anti-Rabbit IgG pAb) | 6 ml | RTU | 2-8℃ |
| 7 | DAB kit (20×) 显色液 | 0.3 ml | RTU | -20℃ |
| 8 | DAB kit (20×) 稀释液 | 0.3 ml | RTU | -20℃ |
| 9 | 复染试剂 | 5 ml | RTU | 室温 |
| 10 | 封片剂 | 5 ml | RTU | 室温 |
| 11 | 对照切片 (人脑) | 1 张 | RTU | 室温 |
| 12 | 说明书 | 1 份 | | |


背景

GFAP (Glial fibrillary acidic protein) is a member of the class III intermediate filament protein family. GFAP is heavily and specifically expressed in astrocytes and certain astroglia of the central nervous system, in satellite cells of peripheral ganglia, and in non-myelinating Schwann cells of peripheral nerves. In addition, neural stem cells strongly express GFAP. Antibodies to GFAP are very useful as markers of astrocytic cells. In addition, many types of brain tumor, presumably derived from astrocytic cells, heavily express GFAP. GFAP is also found in the lens epithelium, Kupffer cells of the liver, in some cells in salivary tumors and has been reported in erythrocytes. GFAP is used as a marker to distinguish astrocytes from other glial cells during development. Mutations in this gene cause Alexander disease, a rare disorder of astrocytes in the central nervous system. Alternative splicing of the GFAP gene results in multiple transcript variants encoding distinct isoforms.

别名

Astrocyte Marker; FLJ45472; GFAP; Glial Fibrillary Acidic Protein; Intermediate filament protein; GFAP_HUMAN.

验证数据

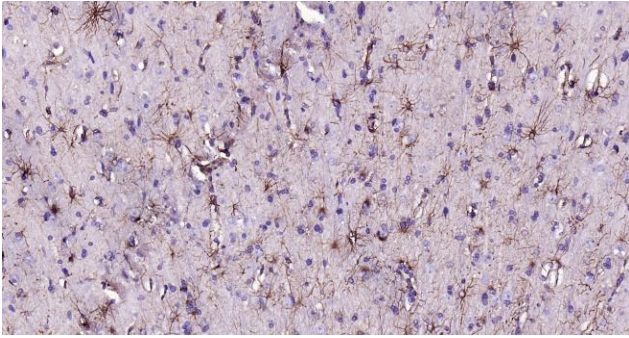

使用 IHC0101H (人胶质纤维酸性蛋白 IHC 试剂盒) 对石蜡包埋的人胶质瘤组织切片进行免疫组化分析。

石蜡包埋组织的免疫组织化学方案

1. 脱蜡水化

石蜡切片置于新鲜二甲苯中浸泡脱蜡 3 次, 每次 15 min; 依次置于不同浓度 (100%、95%、90%、80%、70%) 乙醇浸泡各 5 min, 再置于蒸馏水洗涤 5 min, 重复 3 次。

2. 抗原修复

沸水浴修复: 将 100×**抗原修复缓冲液 (试剂 2)** 用蒸馏水稀释成 1×**抗原修复缓冲液**, 放入修复盒中并提前加热至 95-100℃ (注意盖好以防液体蒸发), 然后将切片放入修复盒中, 在沸水浴环境中保持外沸状态 15 min, 室温自然冷却; 用 **PBS 缓冲液 (试剂 1)**, 将干粉溶解在 2L 蒸馏水中) 清洗 5 min, 重复 3 次。

3. 阻断内源性过氧化物酶

用吸水纸吸去玻片上多余的液体, 用免疫组化笔在组织周围画圈, 加入 2-4 滴**内源性过氧化物酶阻断剂 (试剂 3)**, 室温下置于湿盒中孵育 15 min, 用 PBS 洗涤 5 min, 重复 3 次。

4. 血清封闭

用吸水纸吸去玻片上多余的液体, 加入 2-4 滴**封闭工作液 (试剂 4)**, 置于湿盒内 37℃ 封闭 20 min, 以减少非特异性染色。

5. 一抗孵育

用吸水纸吸去玻片上多余的液体, 加入 2-4 滴**人 GFAP 兔多抗工作液 (试剂 5)**, 置于湿盒中, 4℃ 孵育过夜或 37℃ 孵育 1-2 h。

6. 复温

4℃ 孵育过夜后, 室温下复温 15 min (若在室温下孵育一抗, 则直接进入下一步清洗); 用 PBS 洗涤 5 min, 重复 3 次。

7. 二抗孵育

用吸水纸吸去玻片上多余的液体, 加入 2-4 滴 **HRP 标记羊抗兔 IgG 工作液 (试剂 6)**, 置于湿盒中, 37℃ 孵育 1-2 h; 用 PBS 洗涤 5 min, 重复 3 次。

8. 显色

用吸水纸吸去玻片上多余的液体, 在每张切片上滴加约 50 μL 新配制的 **DAB 工作液 (试剂 7: 试剂 8: PBS=1:1:18)**, 作用 3-5 min。显微镜下观察结果, 达到合适的显色强度后, 用蒸馏水冲洗切片以终止反应, 用蒸馏水冲洗 5 min, 重复 3 次。

9. 复染

滴加适量**复染试剂 (试剂 9)** 复染 3-5 min, 蒸馏水冲洗 5 min, 滴加盐酸酒精分化约 30 s, 蒸馏水洗涤 5 min, 重复 2 次。

10. 脱水封片

将玻片依次置于不同浓度（70%、80%、90%、95%、100%）乙醇，各 5 min；然后置于新鲜二甲苯中浸泡脱蜡 3 次，每次 15 min。用吸水纸吸去多余的二甲苯，滴加适量封片剂（试剂 10）在组织上，将盖玻片盖在组织上，避免产生气泡。

注意事项

1. 建议检测时进行阴性及阳性对照，以提高实验的可靠性。
2. 本品中的配套试剂，请不要用其他生产商产品替换使用。
3. DAB 为致癌物质，请采取必要的防范措施。
4. PBS 洗涤液（试剂 1）配制后在 4℃可保存一周；抗原修复液（试剂 2）及显色剂（试剂 7 和 8）的工作液需每次实验时现用现配。
- *5. 发表论文时引用本产品的写作建议 "IHC0101H, Bioss Antibodies"。引用示例: "Human tissue sections using Human GFAP IHC Kit (IHC0101H, Bioss Antibodies) were stained for GFAP according to the manufacturer's instructions."